


patient commission/configuration ID \_\_\_\_\_



Item	20mm	Description	Potential Problem	Measure	Recommended Inspection, Potential Replacement*	Latest Replacement after
<b>System Joint</b>						
1	SB1069-L0960	bearing nut	wear	replacing	every 6 months	36 months
3	SF0395-02	feather key with pin	breakage	replacing	every 6 months	36 months
4	GS2611-040	sliding washer, Ø = 26mm	wear	replacing	every 6 months	18 months
4	GS2611-045					
4	GS2611-050					
4	GS2611-055					
4	GS2611-060					
5	SH0465-L/AL	cover plate, left lateral or right medial**	wear	replacing	every 6 months	36 months
5	SH0465-R/AL	cover plate, left medial or right lateral**				
6a	VE3771-09/15	O-ring for securing the alignment screw**	wear	replacing	every 6 months	18 months
6c	FE1027-01	pressure spring**	wear	replacing	every 6 months	18 months
6d	GS1108-500	sliding bushing**	wear	replacing	every 6 months	18 months
6e	VE3771-012/26	O-ring damper**	wear	replacing	every 6 months	18 months
6f	SH0493-01	plunger**	wear	replacing	every 6 months	36 months
7a	VE3771-125/15	O-ring for securing the alignment screw**	wear	replacing	every 6 months	18 months
7c	VE3771-07/10	O-ring for securing the motion limiting screw**	wear	replacing	every 6 months	18 months
8	SC1405-L14	countersunk flat head screw with hexalobular socket**	wear	replacing	every 6 months	36 months
9	SC1406-L14	countersunk flat head screw with hexalobular socket (axle screw)**				
5-9	SH4975-L/AL	functional unit plug + go modularity, left lateral or right medial***	loss of function, wear	replacing	every 6 months	36 months
5-9	SH4975-R/AL	functional unit plug + go modularity, left medial or right lateral***				

patient commission/configuration ID \_\_\_\_\_

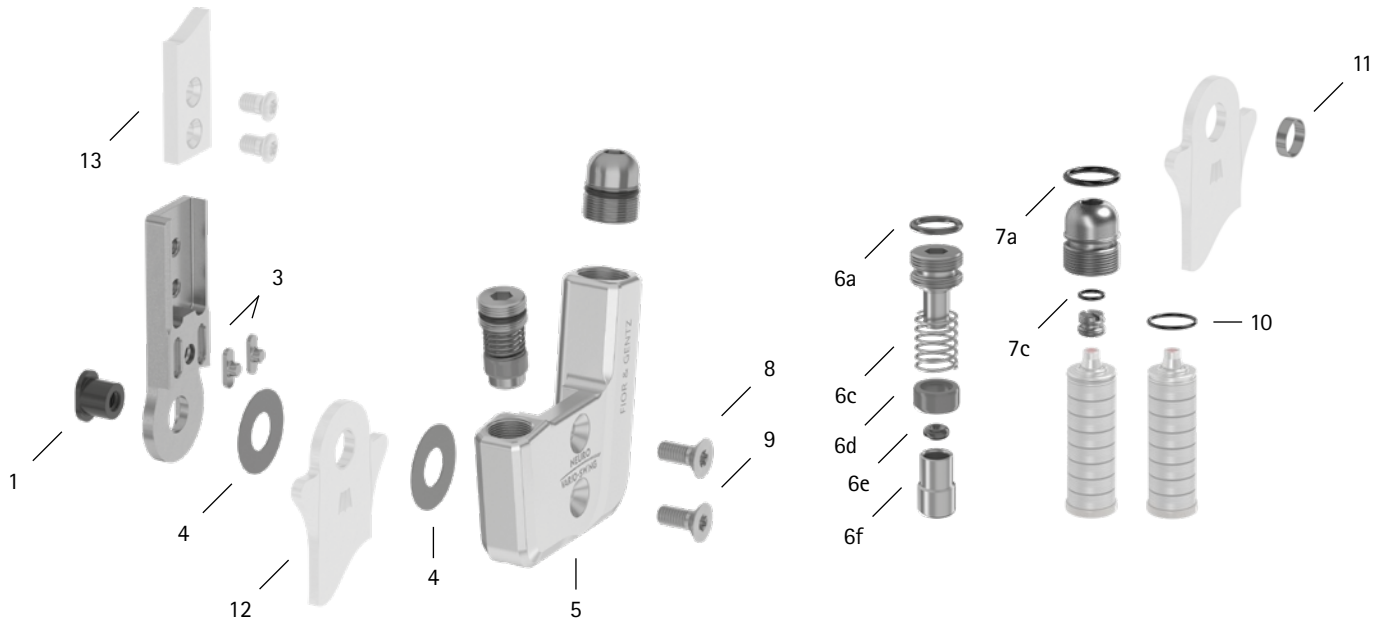

Item	20mm	Description	Potential Problem	Measure	Recommended Inspection, Potential Replacement*	Latest Replacement after
Spring Units						
10	VE3771-11/10	O-ring for securing the spring unit	wear	replacing	every 6 months	18 months
-	SF5805-15/18	spring unit, blue, normal, max. 15° range of motion	wear	replacing	every 6 months	18 months
-	SF5805-15/25	spring unit, green, medium, max. 15° range of motion	radial move of disc springs	realigning disc springs with pliers		
-	SF5805-10/40	spring unit, white, strong, max. 10° range of motion	noise of spring unit with coil spring	greasing the coil spring with orthosis joint grease or spray oil (article no. FT3000-15)		
-	SF5805-10/60	spring unit, yellow, very strong, max. 10° range of motion	noise of spring unit with disc springs	greasing disc springs laterally with spray oil (article no.: FT3000-15)		
-	SF5805-05/99	spring unit, red, extra strong, max. 5° range of motion				
System Stirrups, System Anchors and System Side Bars						
11	BR1211-L030	sliding bushing	wear	replacing	every 6 months	18 months
12	see catalogue	system stirrup	wear or breakage	replacing	every 6 months	48 months
13	see catalogue	system anchor and system side bar	wear or breakage	replacing	every 6 months	if required

\* depending on the assessment of the distributor of the custom-made product regarding the patient's usage behaviour  
\*\* is part of the functional unit  
\*\*\* included system components can be exchanged separately